

Rajasthan Medical Services Corporation Limited, Jaipur

Gandhi Block, Swasthya Bhawan, Tilak Marg, C-Scheme, Jaipur - 302005

Ph. No. 0141-2223887, Fax : 0141-2228065

E-mail : edepmrmisc-ri@nic.in

CIN:U24232RJ2011SGC035067

Website:www.rmisc.nic.in

No. F-8()RMSC/EPM/M-2/2015-16/NIB-165/ 4901


Dated: 18/11/16

All Principal, Medical Colleges,
All the Superintendent of Medical College & Attached Hospitals.
Director (PH/HA/IEC/AIDS/RCH)

Sub:- Approval/Purchase of Store Item **Deep Freezer (Large 500 Ltr.)**, for the rate contract ending on 31.05.2018

Please find enclosed herewith approved firm and rates etc. in respect of Item **Deep Freezer (Large 500 Ltr.)** for the rate contract ending on 31.05.2018 The Rate Contract and its terms & conditions are also available on Rajasthan Medical Services Corporation Ltd., Website www.rmisc.nic.in.

In reference to above Rate Contract No.F-8()RMSC/EPM/M-2/2015-16/NIB-165/...4900
Dated: ...18/11/16 the supplier has executed the agreement with RMSC, as enclosed here for your information & necessary action.



Executive Director (EPM)
RMSCL, Jaipur


No. F-8()RMSC/EPM/M-2/2015-16/NIB-165/ 4901

Dated: 18/11/16

Copy forwarded to the following for information & necessary action:

1. P.S. to Hon'ble Health Minister, Medical & Health Deptt. Govt. of Rajasthan.
2. P.S. to PHS, Medical Health & FW Deptt. Rajasthan, Jaipur.
3. P.S. to Mission Director NHM Jaipur.
4. Director, (PH)/(Aids)/(FW)/(RCH)/(IEC)/(ESI).
5. Principal, Medical College, Ajmer, Bikaner, Jaipur, Jodhpur, Kota, Jhalawar & Udaipur.
6. Principal R.U.H.S. College of Dental Science Jaipur.
7. Principal, RUHS College of Medical Scinces, Jaipur.
8. Superintendent Japuriya Hospital Jaipur (Associated with RUHS College of Medical Scinces, Jaipur).
9. Superintendent, SMS Hospital, Zenana Hospital, Mahila Chikitsalya, Mental Hospital, J.K. Lon Hospital, T.B & Chest Hospital, Jaipur.
10. Superintendent Associated Group of Hospital-Ajmer, M.G. Hospital, Jodhpur, Ummaid Hospital- Jodhpur, PBM Hospital-Bikaner, MBS Hospital-Kota & A.G. Hospital-Udaipur.
11. Director, Medical & Health Services (ESI), Mobile Surgical Unit, Raj. Jaipur.
12. Addl. Director, Medical & Health Services (PW)/(RH)/(Hospital Admn.)
13. Joint Director, Medical & Health Services, (Zone) Jaipur, Ajmer, Udaipur, Jodhpur, Bikaner, Kota & Bharatpur.
14. All P.M.O.'s.
15. All CM&HO's.
16. All Dy. CM&HO's.
17. AGM (IT), RMSC, Jaipur
18. M/s Remi Elektrotechnik Limited, Remi House, 11 Cama Indl. Estate, Goregaon (E), Mumbai-400 063, India.
19. Guard file.


Executive Director (EPM)
RMSCL, Jaipur

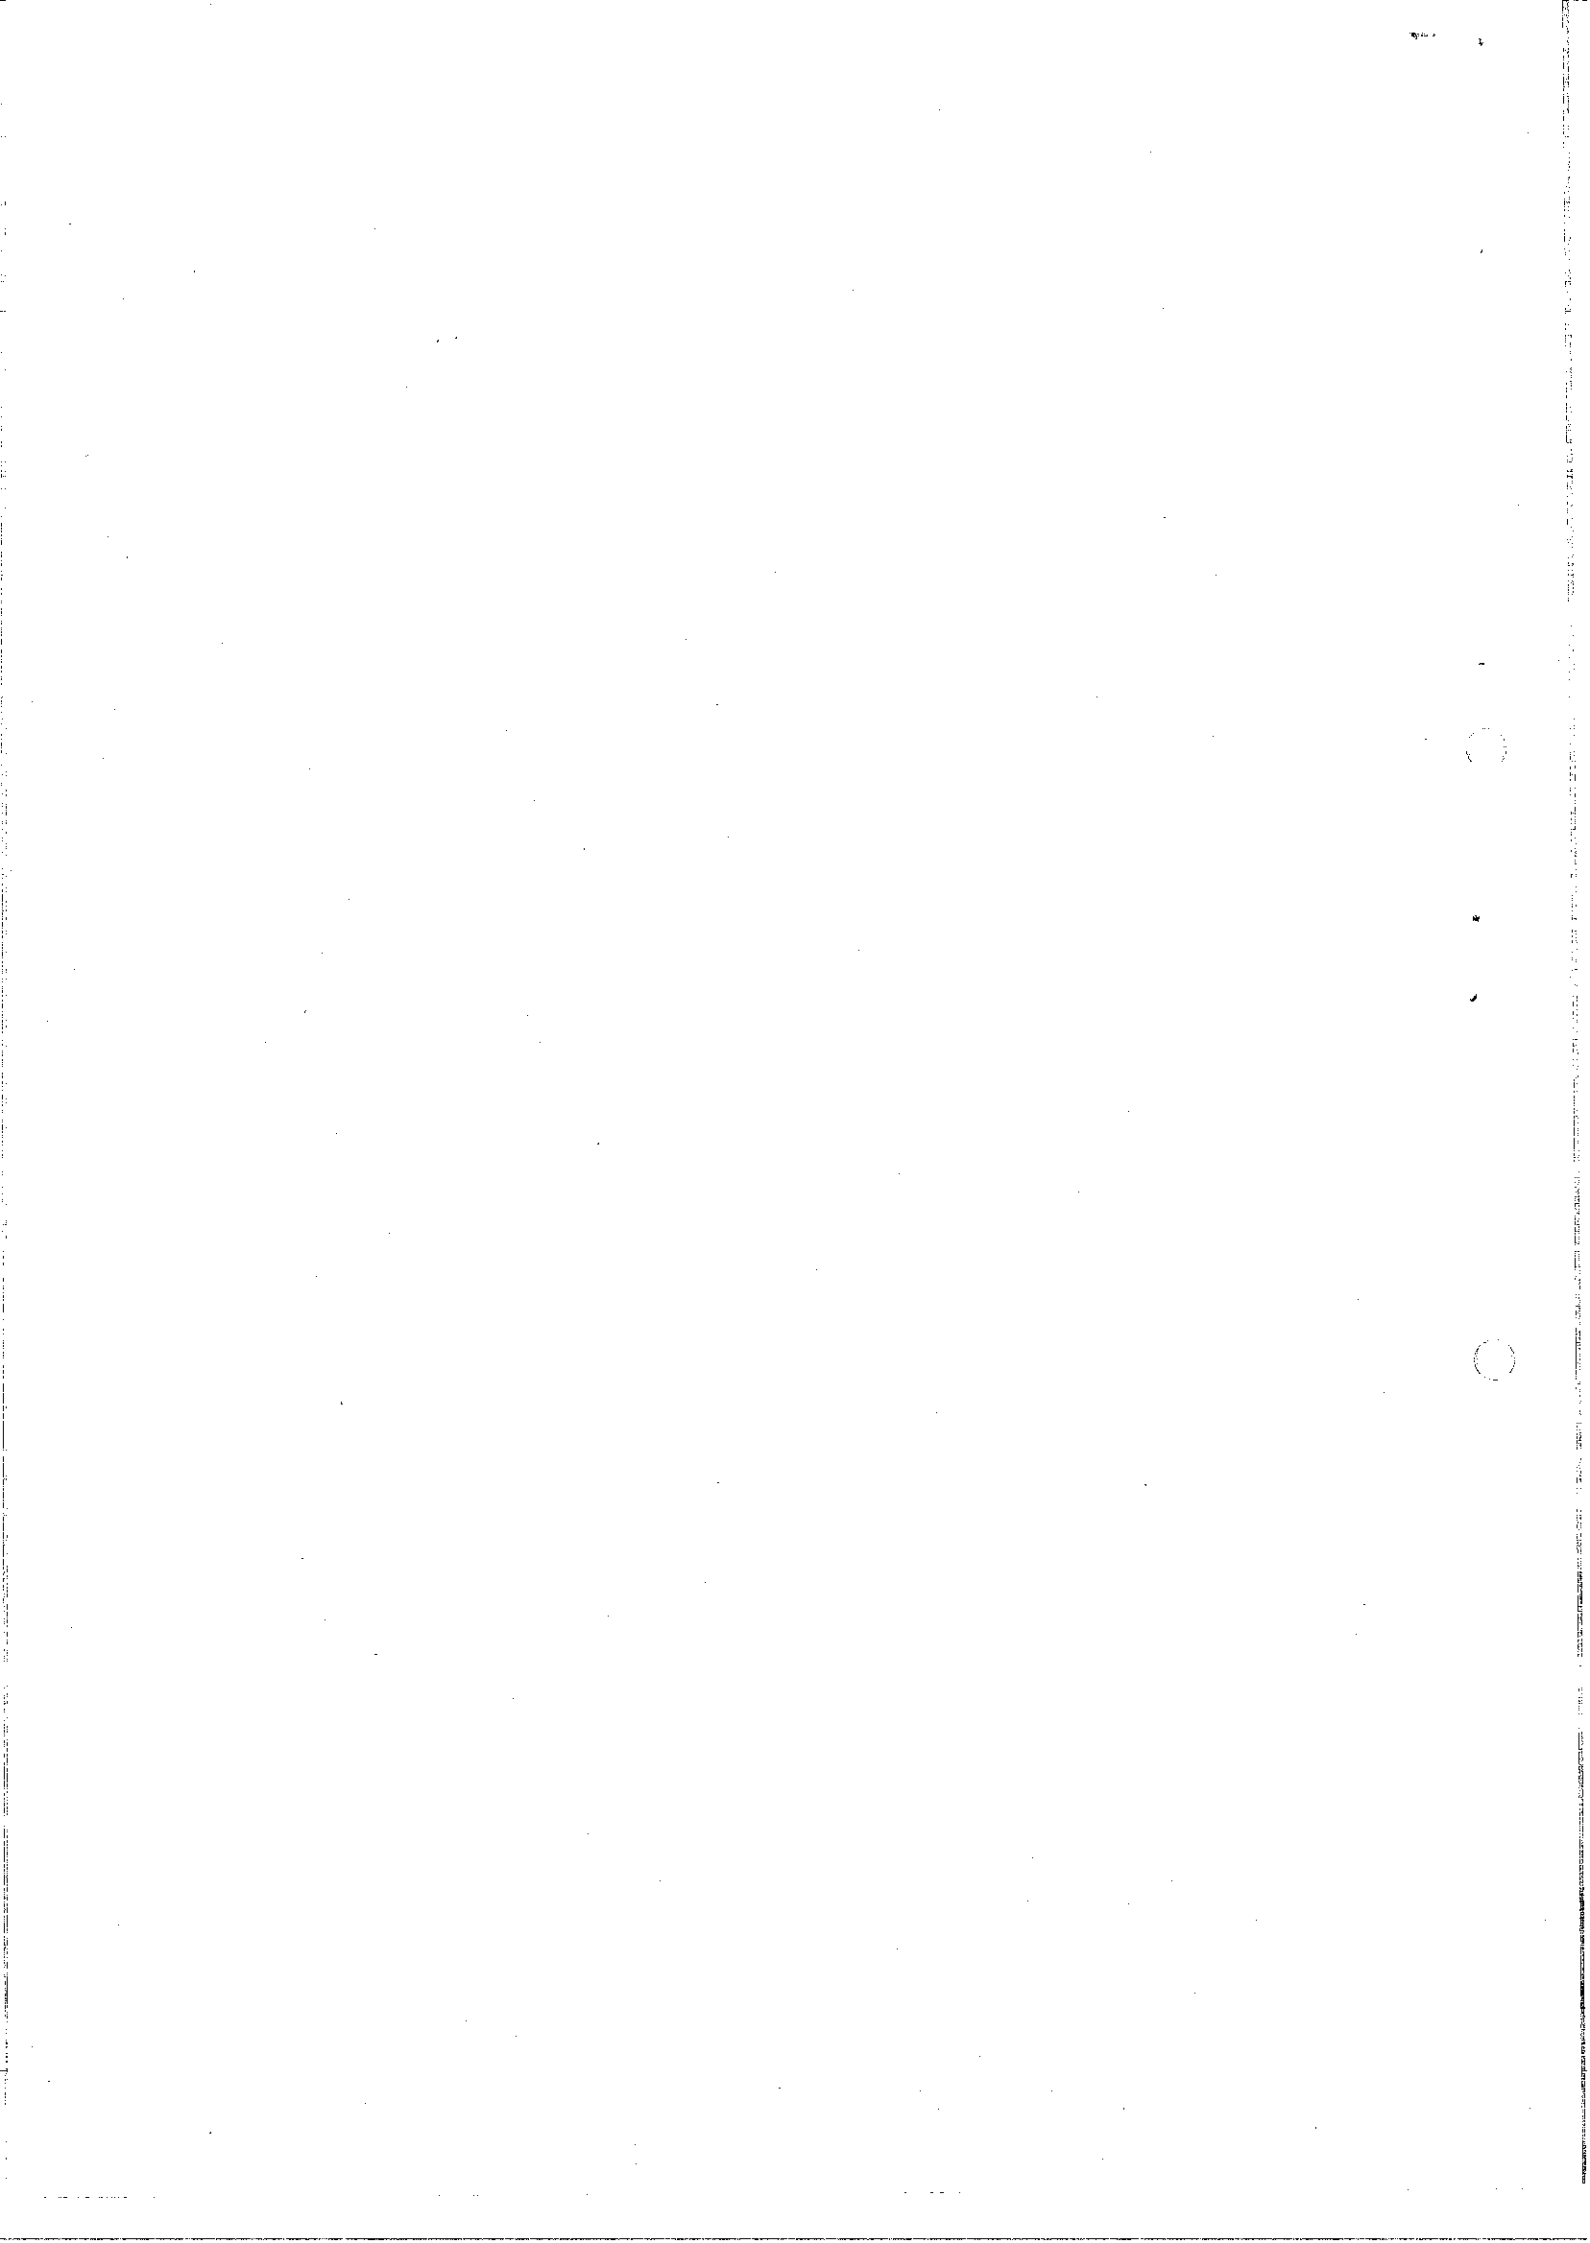

Rajasthan Medical Services Corporation Limited, Jaipur

Gandhi Block, Swasthya Bhawan, Tilak Marg, C-Scheme, Jaipur - 302005

Ph. No. 0141-2223887, Fax : 0141-2228065

E-mail : edepmrmssc-ri@nic.in

CIN:U24232RJ2011SGC035067

Website:www.rmssc.nic.in

No. F-8()RMSC/EPM/M-2/2015-16/NIB-165/ 4900

Dated: 18/11/16

Rate Contract and Price details

S.N.	Item	Detail
1.	Name of Equipment / Item	Deep Freezer (Large 500 Ltr.)
2.	Name & Address of Firm	M/s Remi Elektrotechnik Limited, Remi House, 11 Cama Indl. Estate, Goregaon (E), Mumbai-400 063, India, E-Mail:- bids@remilabworld.com
3.	Brand/ Model / Make	REMI / RQF-425
4.	Packing Unit	One
5.	R/C No. & Validity	R.C. No. 345 (Valid up to 31.05.2018)
6.	Net Rate Per packing Unit (Rs.)	Rs 73,125.00 (In Words, Rs. Seventy Three Thousand One Hundred Twenty Five Only) + 2% concessional CST against C-form
7.	Taxes Concessional CST @ 2% (Rs.)	Rs. 1,462.50
8.	RMSC Surcharges @ 5%	Rs. 3,729.38
9.	Total Price (Rs.)	Rs. 78,316.88
10.	Guarantee Period	2 years
11.	CMC after Guarantee Period	3 years
12.	<u>Specifications of item Deep Freezer (Large 500 Ltr.)</u>	
	<p>1. Description of Function:</p> <p>(i) Deep Freezers maintain temperatures (-) 25°C to (-) 15°C, to store fruits & vegetable / Meat and /or freeze ice packs.</p> <p>(ii) Deep Freezers are required at district and regional levels, to store Food Samples and prepare ice packs required for passive cooling in food sample carriers and cold boxes.</p> <p>2. Operational Requirements:</p> <p>(i) Designed for tropical climates Temperature up to 45 degree centigrade.</p> <p>(ii) Target holdover time should be not less than 2 hrs and 30 minutes.</p> <p>(iii) Hot and Cold compressors starting at 172 volts (22% below rated voltage).</p> <p>(iv) Manufacturing process of the product should not use or produce hazardous chemicals-gases.</p> <p>(v) Provision for drainage for the waste water.</p> <p>(vi) Should have legs in the base with rotating screw type height adjustments to balance the weight on uneven floor.</p> <p>(vii) The unit should have ground clearance minimum 100 mm.</p> <p>3. Technical Specifications:</p> <p>(i) Gross Volume: 450- 500 Litres.</p> <p>(ii) Construction: Internal: Stainless 304 grade steel/ Aluminum body. External: Corrosion Resistance</p> <p>(iii) Chest Type with CFC-free insulation.</p> <p>(iv) Solid door with lock handle.</p> <p>(v) Type: Compression Cycled, CFC Free (both for refrigeration and insulation) All system tubing (suction tube, freezer tube and condensing tube) should be of good quality pure copper coil.</p> <p>(vi) Temperature of compartment to be maintained between (-) 25°C to (-) 15°C continuous availability of energy at ambient temperatures 5 to 45 °C.</p> <p>(vii) Inlet of Capillary should be outside the PUF body.</p> <p>(viii) ON/OFF Switch and power indicator should be available.</p> <p>(ix) A microprocessor based control unit should be provided for setting of temperature and</p>	

✓ 22 8

display following features:

- (a) 3 digit display (to one decimal point) of cabinet temperature. The sensor should be placed 25 to 50 mm above base of chamber.
- (b) Power indicator.
- (c) Audio (minimum 65dBA) and visual alarm against the violation of set temperature range.
- (d) Min. & Max. Cabinet temperature digital display of last 24 hrs. and breaches during last 24 hrs.
- (e) The Unit should be sealed protected from dust, moisture or condensed water falling over it
- (f) Accuracy for digital controller ± 0.5 degree centigrade.

4. System Configuration

- (i) Programmable Micro-processor control unit with child lock facility.
- (ii) Should have provision to set minimum and maximum temperature at 0.1 degree Centigrade to programme the unit for continuous operation.
- (iii) Should have provision for defrosting program.

5. Accessories, spares

- (i) fruits & vegetable / Meat storage basket allowing free circulation of air, having the size to be able to accommodate 4 to 6 of them in the unit and suitable to match the net volume requirement. It should be minimum 5 wire basket.
- (ii) The supplier is required to maintain all the spare parts throughout the guarantee period and not less than ten years.

6. Environmental Factors:

- (i) The unit should be capable of being stored continuously in ambient temperature of 0 to 50 deg C and relatively humidity of 95%.
- (ii) The unit shall be capable of operating continuously in ambient temperature of 5 to 45 deg C and relative humidity of 90%.
- (iii) The plug should be flexible and unbreakable sealed rubber type.

7. Power Supply

- (i) Power Input to be 220-240 VAC, 50 Hz as appropriate fitted with Indian plug.
- (ii) **Voltage Stabilizer should be supplied** as per the quoted Deep freezer requirement.

8. Standards and Safety

- (i) **Product should be CE approved.**

9. Documentation:

- (i) A paper copy of user/operator manuals to be supplied in English.
- (ii) A paper copy of technical/wiring diagram/maintenance manuals to be supplied in English.
- (iii) **Certificate of Testing should be submitted at the time of supply from NABL certified lab / ILAC/ STQC Labs.**

10. Packing of the equipment during shipment:

- (i) The supplier should provided strong and sufficient packing to ensure safe arrival of goods at the destination free from loss or damage.
- (ii) A vertical arrow should be marked at all sides of packages to ensure transportation of equipment in vertical position. TOP and BOTTOM should also be written.
- (iii) To put label and signage's for HANDLE WITH CARE on all sides of the crates as per - packing & shipment norms.

Terms & Conditions

1. Guarantee: **Two years** on equipment from the date of installation.
2. CMC: CMC will be given @5% (of net rate-inclusive of Excise Duty & exclusive of VAT/CST etc.) plus service tax (as applicable) and yearly escalation of 5% on last year's CMC price. The CMC may be awarded for three years (on yearly basis) after completion of guarantee period of two years.
3. Installation and Training will be done by the supplier free of cost.
4. The service engineer should be based in Rajasthan.
5. The company should mention the make and model name/number of the quoted equipment and submit the technical brochure of the quoted model in the technical compliance sheet as per technical specifications.

2/10 20

13. Comprehensive Maintenance Contract Charges (per year/per machine)

Rates (Rs.) Per Unit	First Year	Second Year	Third Year	Fourth Year	Fifth Year
Comprehensive Maintenance Agreement (CMA)	CMC: CMC will be given @5% (of net rate-inclusive of Excise Duty & exclusive of VAT/CST etc.) plus service tax (as applicable) and yearly escalation of 5% on last year's CMC price. The CMC may be awarded for three years (on yearly basis) after completion of guarantee period of two years.				


Executive Director (EPM)

Rajasthan Medical Services Corporation Ltd.,
Jaipur



