

Rajasthan Medical Services Corporation Limited, Jaipur

Gandhi Block, Swasthya Bhawan, Tilak Marg, C-Scheme, Jaipur - 302005

Ph. No. 0141-2223887, Fax : 0141-2228065

E-mail : edepmrmisc-ri@nic.in

CIN:U24232RJ2011SGC035067

Website:www.rmesc.nic.in

No. F-8(109) RMSC/EPM/M-1/B.A. 113.4/NIB-226/2017/381

Dated: 12/9/17

Order For Rate Change In Rate Contract Due To GST Provision

S.No.	Item	Detail
1.	Name of Equipment / Item	Horizontal Laminar Air Flow
2.	Name & Address of Firm	M/s Authentic Instruments 31, RIICO Industrial Area Jhotwara, Kamani Choraha Jaipur- 302012 E-mail: support@authenticinstruments.com calibration@authenticinstruments.com
3.	Brand/ Model / Make	Authentic/HLAF
4.	Packing Unit	Each
5.	R/C No. & Validity	No. F-8(109) RMSC/EPM/M-1/B.A. 113.4/NIB-226/2017/1769 Dated: 21.04.17 R.C. No. 381 (Valid up to 30.04.2019)
6.	Net Rate Per packing Unit (Rs.)	Rs. 99,000.00
7.	Taxes	Rs. 0.00 (VAT is Exempted)
8.	RMSC Surcharges @ 5%	Rs. 4950.00
9.	Total Rate Including Tax And RMSC Surcharges	Rs. 1,03,950.00
10.	Basic New Rate (HSN Code-9018)	
	(i) Existing Approved Net Rate	= Rs 99000.00/-
	(ii) Less Excise Duty	= Nil
	(iii) Less any other amount intimated by the firm	= Nil
	(iv) New Basic Rate {(i)-(ii)-(iii)}	= Rs. 99000.00/-
11.	Revised Rates for supply to RMSC from Suppliers	
	(i) New Basic Rate	= Rs. 99000.00/-
	(ii) IGST	= Nil
	(iii) CGST @ 6%	= 5940.00/-
	(iv) SGST @ 6%	= 5940.00/-
	(v) Approved Rate For Supplier To RMSC {(i)+(ii)+(iii)+(iv)}	Rs. 110880.00/-
12.	Revised Rate For Supply to Consignee From RMSC	
	(i) New Basic Rate	= Rs 99000.00/-
	(ii) RMSC Surcharge@5% On (i)	= Rs. 4950.00/-
	(iii) CGST @ 6%	= Rs. 6237.00/-
	(iv) SGST @ 6%	= Rs. 6237.00/-
	(v) Grand Total Rate For consignee	= Rs. 116424.00/-

2.12
Executive Director (EPM)

Rajasthan Medical Services Corporation Ltd.,
Jaipur

No: F-8(109) RMSC/EPM/M-1/B.A. 113.4/NIB-226/2017/.....


Dated:.....

Copy forwarded to the following for information & necessary action:

1. P.S. to Mission Director NHM Jaipur.
2. Director, (PH)/(Aids)/(FW)/(RCH)/(IEC)/(ESI).
3. Principal, Medical College, Ajmer, Bikaner, Jaipur, Jodhpur, Kota, Jhalawar & Udaipur.

- ✓
4. Superintendent Japuriya Hospital Jaipur (Associated with RUHS College of Medical Sciences, Jaipur).
 5. Director, Medical & Health Services (ESI), Mobile Surgical Unit, Raj. Jaipur.
 6. All P.M.O.'s.
 7. All CM&HO's.
 8. Executive Director (Logistics/Finance)
 9. AGM (IT), RMSC, Jaipur
 10. All DPC's DDW Rajasthan
 11. M/s Authentic Instruments 31, RIICO Industrial Area Jhotwara, Kamani Choraha Jaipur
 12. Guard file.

27
Executive Director (EPM)
Rajasthan Medical Services Corporation Ltd.,
Jaipur

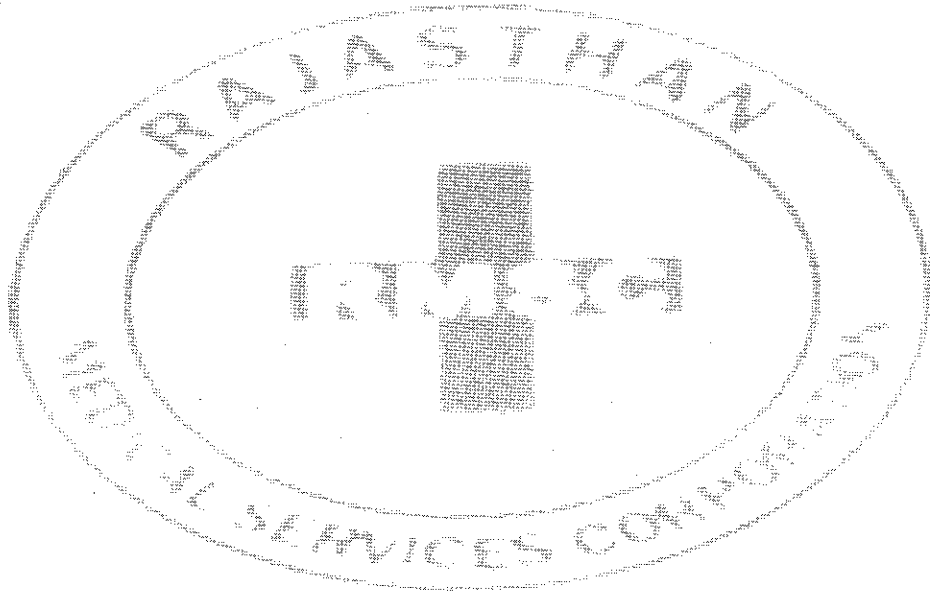

॥ सर्वे सन्तु निरामयाः ॥

Technical Specifications of item Horizontal Laminar Flow

1. Construction-fabricated from welded 16 gauge C.R. steel includes adjustable levellers.
2. Work surfa
3. ce: 304 stainless steel.
4. Finish: exterior surface feature a chip-resistant, powder-coated finish of approximately 0.6 mm thickness.
5. Front panel: movable transparent scratch resistant sheet of approx. 6mm thickness.
6. Pre-filters: disposable fiber glass with Filtration efficiency of 98% for all types of particles of size 8 micron and larger.
7. HEPA filter: choice of HEPA (rated 99.97% efficient@ 0.3µm particles) or ULPA (rated 99.99% efficient@0.12µm particles)
8. Lighting: Fluorescent type with lux > 800 & UV light.
9. On and OFF timer indicator for UV light along with total time usage of UV light.
10. Work table size 4' x 2' x 3.5' (W x D x H) in feet tolerance ±5%
11. FFU airflow: 650 CFM (2" x 4"), 460 (2" x 3") of air at filter pressure drop from 0.35-0.795" W.G at 90 FPM.
12. On site annual calibration and validation.
13. On site counting of dust particles in laminar air flow chamber annually under guarantee.
14. Provision of hanging the blood bag in cabin during preparation of components.
15. Installation commissioning and trial run will be the responsibility of the supplier.
16. Appropriate manometer to measure the pressure should be provided along the equipment.
17. The system should be CE approved (Valid documentation should be submitted in technical bid).
18. Manufacturing should be compliant with ISO 13485 (Valid documentation should be submitted in technical bid).
19. **Guarantee:** Two years on equipment from the date of installation.
20. **CMC:** CMC will be given @ 5 % (of net rate - inclusive of Excise Duty & exclusive of VAT / CST etc.) Plus service tax (as applicable) and yearly escalation of 5 % on last year's CMC price. The CMC may be awarded for five years (on yearly basis) after completion of Guarantee period of two years.
21. The company should submit technical compliance sheet as per technical specifications mentioning the make & model of quoted item along with catalogue in the Technical bid .
22. Installation will be done by supplier free of cost.
23. The service engineer should be based in Rajasthan.
24. Four Preventive Maintenance services annually during Guarantee and CMC period are essential.
25. Demonstration of equipment is must for final technical approval.

Comprehensive Maintenance Contract Charges (per year/per machine)

Rates (Rs.) Per Unit	First Year	Second Year	Third Year	Fourth Year	Fifth Year
Comprehensive Maintenance Agreement (CMA)	CMC: CMC will be given @ 5 % (of net rate - inclusive of Excise Duty & exclusive of VAT / CST etc.) Plus service tax (as applicable) and yearly escalation of 5 % on last year's CMC price. The CMC may be awarded for five years (on yearly basis) after completion of Guarantee period of two years.				